



Urinalysis for diaper-wearing elderly people using a combination of cotton-based diagnostic devices and smartphone-based image analysis

Wei-Hsuan Sung¹, Chao-Min Cheng²

¹College of Medicine, Chang Gung University and Chang Gung Memorial Hospital Linkou Medical Center, Taoyuan, Taiwan; ²Institute of Biomedical Engineering, National Tsing Hua University, Hsinchu, Taiwan

Contributions: (I) Conception and design: All authors; (II) Administrative support: All authors; (III) Provision of study material or patients: All authors; (IV) Collection and assembly of data: All authors; (V) Data analysis and interpretation: All authors; (VI) Manuscript writing: All authors; (VII) Final approval of manuscript: All authors.

Correspondence to: Chao-Min Cheng. Institute of Biomedical Engineering, National Tsing Hua University, No.101, Sec. 2, Guangfu Rd., East Dist., Hsinchu City 300, Taiwan. Email: chaomin@mx.nthu.edu.tw.

Background: Urinary tract infection (UTI) is one of the most common bacterial infections, annually affecting 150 million people worldwide. The highest prevalence of UTI in the overall elderly population. However, practical problems have occurred in urine sampling in diaper-wearing elderly people. Our aim is to develop a new type of the *in-vitro* diagnostic devices based on “cotton”, which allows us to detect the nitrite concentrations in urine (i.e., biomarker for urinary tract infection). The combination of cotton-based diagnostic device and a smartphone-based image analysis would help the healthcare people early diagnose urinalysis-based diseases such as UTI, and improve the life quality in elderly populations around the world.

Methods: Our diagnostic device integrated into diaper is made up with three primary parts: a test pad, a flow channel made by hydrophobic and hydrophilic cotton and plastic packaging substrates. The smartphone-based image analysis (a specific APP) solved recording issues including variances in either light or focal distance. The mean value was calculated and analyzed based on 8-bit grayscale using ImageJ software and defined as $255 - [\text{experiment zone intensity}]$.

Results: The nitrite test color changes from colorless to purple, correlating positively to concentration (from 0.156 to 5 μM) in both test paper only and test pad integrated with diaper and the mean value is calculated and analyzed.

Conclusions: Since this device is inexpensive, portable, simple, structurally integrating with diapers and functionally integrated with the smartphone-based application, it would have a wide range potential of becoming a commercially viable diagnostic system, in particular, for the daily healthcare of elderly people.

Keywords: Biosensors; geriatric care; urinary tract infection (UTI); smartphone-based colorimetric readout

Received: 11 February 2019; Accepted: 15 August 2019; Published: 03 September 2019.

doi: 10.21037/ht.2019.08.02

View this article at: <http://dx.doi.org/10.21037/ht.2019.08.02>

Introduction

Urinary tract infections (UTI) are one of the most common bacterial infections, annually affecting 150 million people worldwide (1). In 2010, the direct and indirect costs of UTI in the United States amounted to

approximately \$2.3 billion (2). The incidence of UTI in women is far higher than in men. This can be explained by the following two reasons: (I) the shorter female urethra allows colonized bacteria to reach the bladder more easily; and, (II) the female urethral opening is very close to the

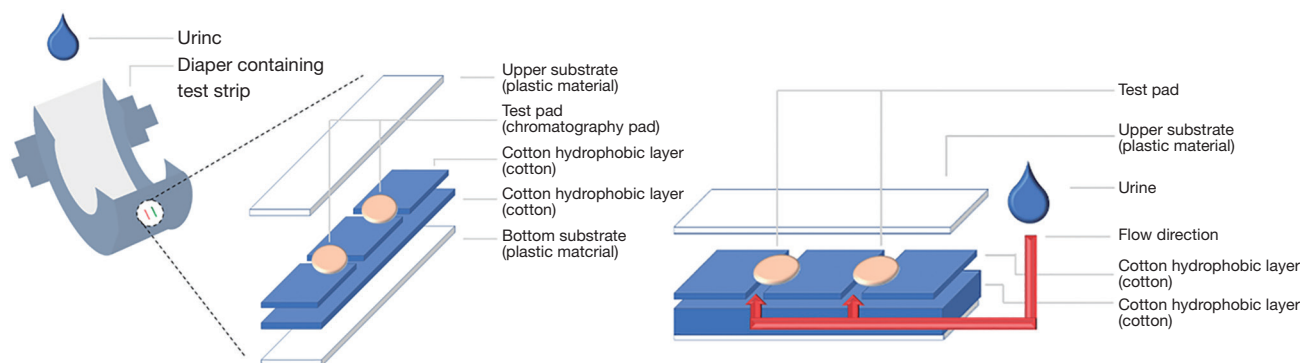


Figure 1 Schematic of a disposable diaper structure integrated with our urine test device and a cross-section of the test paper. The sample flow direction (red line) is indicated.

rectum, which facilitates bacterial migration (3).

Despite the higher incidence among women, the highest prevalence of UTI is actually in the overall elderly population. UTI strongly influences not only community-dwelling older adults but also highly functionally impaired long-term care facilities residents (4). Currently, the diagnosis of UTI is based on the presence of clinical symptoms in combination with positive urine culture results. Unfortunately, the evaluation of urinary symptoms among elderly patients is extremely challenging. First, symptoms of UTI are highly variable in elderly adults, nonspecific to infection. Second, practical problems have occurred in urine sample collection, resulting in inappropriate laboratory results interpretation (5). Furthermore, the diagnosis of symptomatic UTI in older adults with associated disorders such as Alzheimer's disease, Parkinson's disease, and stroke is even more challenging (6). Elderly patients suffering from functional or cognitive impairments have great difficulty communicating localized genitourinary symptoms, which can include dysuria, frequency, urgency, suprapubic pain, or hematuria (3).

Given that increased age is associated with higher risk of septic shock, there is an urgent need for a new device for bacteriuria screening and early UTI diagnosis among patients aged 65 years or older (7). We took the approach of designing a device that would facilitate more timely and appropriate antibiotic treatment that could both hasten recovery and counter the trend toward worldwide antibiotic resistance from therapeutic misuse. With innovations in cellphone-based technologies during the last decade, there are considerable advances in point-of-care testing

(POCT) devices (8,9). In this study, our aim is to develop an inexpensive, easy to use, rapid, and accurate cotton-based *in-vitro* diagnostic device (IVD) to detect nitrite concentrations.

Methods

Cellulose-based materials (e.g., paper, cotton and nitrocellulose) have been widely used for both qualitative and quantitative medical diagnostics (e.g., dengue fever and VEGF level) (10,11). Among these naturally-derived materials, cotton provides good flexibility and biocompatibility that facilitate the creation of highly suitable diagnostic devices.

Our diagnostic device comprises three primary parts: (I) a test pad (Whatman chromatography paper); (II) a flow channel made by hydrophobic and hydrophilic cotton (Shiseido cleansing cotton); and, (III) upper and lower plastic packaging substrate (12). Wax printing was used to create complete hydrophobic barriers around test zones. We attached the three part together to make the device. The flow channel allowed fluid to pass removing impurities. This particular urine testing device was integrated directly into a diaper with one side facing the patients' body, and the reverse side adhered onto the diaper (Figure 1). We converted the colorimetric results to 8-bit grayscale using ImageJ software and defined color intensity as 255-[experiment zone intensity].

Diapers are useful for sample collection in urinalysis, especially when patients suffer from urinary incontinence. Commonly, the urine sample is collected by

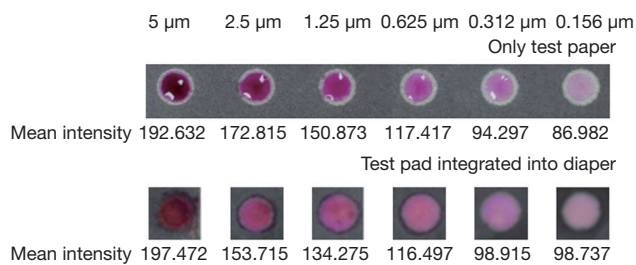


Figure 2 Colorimetric readouts of various nitrite concentrations in both test paper only and test pad integrated with diaper. The colorimetric results was converted to 8-bit grayscale using ImageJ software and the color intensity was defined as $255 - [\text{experiment zone intensity}]$.

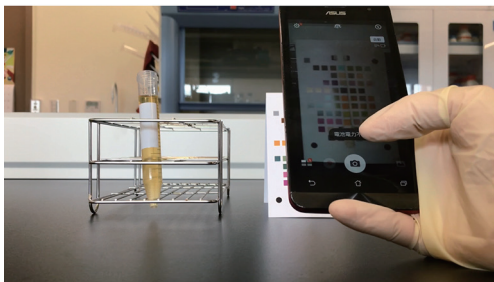


Figure 3 Colorimetric readouts by using a comparator card with the incorporation of the smartphone-based application (APP) to obtain more accurate results.

catheterization in these cases, contributing to pain and sample contamination (13). By combining a diagnostic device with a diaper, urine samples are collected immediately, reaching test pads through capillary flow. The entire procedure is completed in a single step.

Results

To evaluate the performance of urine test device to detect nitrite, we spotted serially diluted nitrite onto each test zone. The nitrite test color change was from colorless to purple, and the colorimetric reaction was photographed through using a smartphone camera. *Figure 2* shows that samples with different nitrite concentrations have a visually distinguishing color intensity that correlates positively to concentration (from 0.156 to 5 μM) in both test paper only and test pad integrated with diaper.

We used a smartphone as a recording device to obtain

and analyze the colorimetric-based images when the colorimetric responses occurred in the test pad. The red green blue (RGB) information was then provided accordingly. As a result, we conducted the accurate color analysis by using a comparator card with the known RGB values. We applied our smartphone-based application (APP) as well for timely image analysis (*Figure 3*). The results became more sensitive and specific once we incorporated the machine learning algorithm.

Discussion

Conventional methods have been widely used to detect bacteria in urine include urine dipsticks and urine culture. The dipsticks are economical with the minimal equipment required; however, they require a relatively large amount of sample (14). The urine culture is considered as a gold standard, to provide the quantitative results but it incurs a fair amount of cost, and time (between 24 and 48 hours). The diagnosis and the following treatment of urinary tract infection are delayed, leading to severe morbidity and mortality.

In comparison to conventional diagnostic methods, our cotton-based device features the following advantages: (I) it detects clinical target in a single step using one device, carrying a lower possibility of clinical sample contamination; (II) it avoids sensitivity and precision issues encountered by the use of unpurified samples in clinical analysis. The design of our device uses chromatography paper and cotton material to create a fluid channel that dilutes concentration and filters unpurified samples before they are absorbed by the chromatography test pad. Notably, this tool may offer significant advantages for diagnostic testing in a variety of arenas including rural/remote areas and long-term health care centers. It can also be used in underdeveloped and developing countries where electricity and laboratory facilities are scarce.

Noting the potential for cross-communication between detection pads designed for testing different biomarkers and resulting interference, we used wax printing to create complete hydrophobic barriers around test zones. We recommend clinical trials to improve sensitivity and specificity as well as possible design optimization that may include the addition of other useful biomarkers.

The color-based signal of our assay can be easily detected by either visual interpretation or smartphone

camera (15,16). We have used this approach in a previous study (17). Moving forward, we could optimize the APP for more accurate timely image diagnostics. This device could be optimized through machine learning and potential variance issues with light and focal distance could be solved. The combination of a cotton-based diagnostic device and a smartphone-based APP would significantly contribute to therapeutic advances via early diagnosis, thus improving the quality of life among the elderly across all nations.

In addition to being used among the elderly, this device could be used by infants and pregnant women. Recurrent UTI among infants may be an indicator of congenital urinary tract abnormalities. With the application of our diagnostic device, early diagnosis and initiation of treatment is possible, preventing future renal scarring and end-stage renal disease. Among pregnant women, adaptive changes in the urinary tract during pregnancy predispose them to relatively frequent occurrence of UTIs. Moreover, pregnant women are at higher risk of progressing to upper urinary tract infection (e.g., pyelonephritis) from lower urinary tract infection. UTI during pregnancy may result in severe fetal complications, including preterm labor and low birth weight.

Conclusions

The experimental results indicate that our newly developed diagnostic tool is a useful one-step device for detecting clinical target related to UTI. Because this device is inexpensive, portable, and easy to use, we feel that diapers integrated with this or a similar, optimized diagnostic tool has great potential for development into a commercially viable diagnostic device.

Acknowledgments

Funding: The study was supported by project ‘MOST 108-2745-8-007-001’ of Ministry of Science and Technology, Taiwan.

Footnote

Conflicts of Interest: The authors have no conflicts of interest to declare.

Ethical Statement: The authors are accountable for all

aspects of the work in ensuring that questions related to the accuracy or integrity of any part of the work are appropriately investigated and re-solved. In this study, ethics committee approval and informed consent were not considered to be necessary.

References

1. Flores-Mireles AL, Walker JN, Caparon M, et al. Urinary tract infections: epidemiology, mechanisms of infection and treatment options. *Nat Rev Microbiol* 2015;13:269-84.
2. Foxman B. The epidemiology of urinary tract infection. *Nat Rev Urol* 2010;7:653-60.
3. Geerlings SE. Clinical Presentations and Epidemiology of Urinary Tract Infections. *Microbiol Spectr* 2016;4. doi: 10.1128/microbiolspec.UTI-0002-2012.
4. Nicolle LE. Urinary Tract Infections in the Older Adult. *Clin Geriatr Med* 2016;32:523-38.
5. Detweiler K, Mayers D, Fletcher SG. Bacteruria and Urinary Tract Infections in the Elderly. *Urol Clin North Am* 2015;42:561-8.
6. Rowe TA, Juthani-Mehta M. Diagnosis and management of urinary tract infection in older adults. *Infect Dis Clin North Am* 2014;28:75-89.
7. Hsiao CY, Yang HY, Chang CH, et al. Risk Factors for Development of Septic Shock in Patients with Urinary Tract Infection. *Biomed Res Int* 2015;2015:717094.
8. Vashist SK, Luppia PB, Yeo LY, et al. Emerging Technologies for Next-Generation Point-of-Care Testing. *Trends Biotechnol* 2015;33:692-705.
9. Vashist SK, Mudanyali O, Fau - Schneider EM, Schneider Em Fau - Zengerle R, et al. Cellphone-based devices for bioanalytical sciences. *Anal Bioanal Chem* 2014;406:3263-77.
10. Wang HK, Tsai CH, Chen KH, et al. Cellulose-based diagnostic devices for diagnosing serotype-2 dengue fever in human serum. *Adv Healthc Mater* 2014;3:187-96.
11. Hsu MY, Hung YC, Hwang DK, et al. Detection of aqueous VEGF concentrations before and after intravitreal injection of anti-VEGF antibody using low-volume sampling paper-based ELISA. *Sci Rep* 2016;6:34631.
12. Lin SC, Hsu MY, Kuan CM, et al. Cotton-based diagnostic devices. *Sci Rep* 2014;4:6976.
13. Bertao AR, Tao D. Stability of colorimetric results in the detection of urine biomarkers using a paper-based

- analytical device. *Conf Proc IEEE Eng Med Biol Soc* 2017;2017:185-8.
14. Kayalp D, Dogan K, Ceylan G, et al. Can routine automated urinalysis reduce culture requests? *Clin Biochem* 2013;46:1285-9.
 15. Wu MY, Hsu MY, Chen SJ, et al. Point-of-Care Detection Devices for Food Safety Monitoring: Proactive Disease Prevention. *Trends Biotechnol* 2017;35:288-300.
 16. Yang K, Peretz-Soroka H, Liu Y, et al. Novel developments in mobile sensing based on the integration of microfluidic devices and smartphones. *Lab Chip* 2016;16:943-58.
 17. Tsai TT, Huang CY, Chen CA, et al. Diagnosis of Tuberculosis Using Colorimetric Gold Nanoparticles on a Paper-Based Analytical Device. *ACS Sens* 2017;2:1345-54.

doi: 10.21037/ht.2019.08.02

Cite this article as: Sung WH, Cheng CM. Urinalysis for diaper-wearing elderly people using a combination of cotton-based diagnostic devices and smartphone-based image analysis. *Health Technol* 2019;3:8.